

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**



UV FLUX MULTIPLICATION SYSTEM FOR STERILIZING AIR, MEDICAL DEVICES
AND OTHER MATERIALS

Clark, et al.

Appl. No.: 10/724,017

Atty Docket: NOVTR.002A

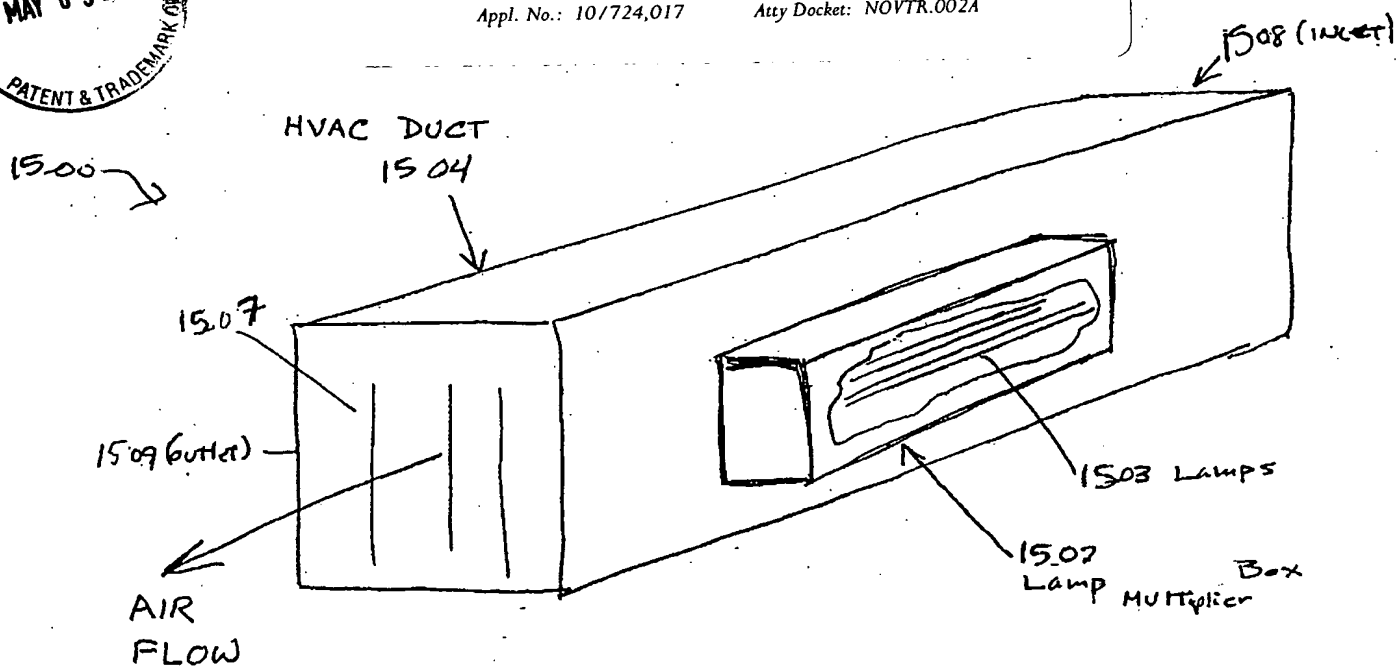


FIGURE 5A


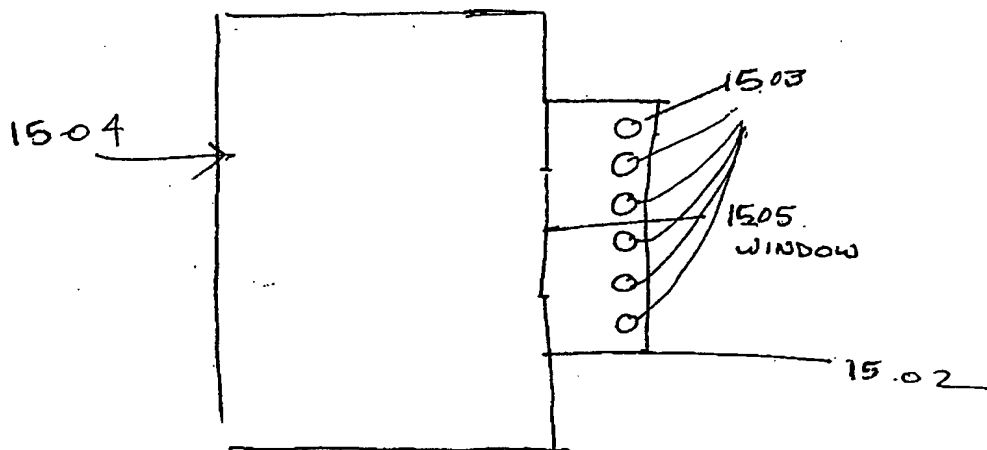


FIGURE 5B



UV FLUX MULTIPLICATION SYSTEM FOR STERILIZING AIR, MEDICAL DEVICES
AND OTHER MATERIALS

Clark, et al.

Appl. No.: 10/724,017

Atty Docket: NOVTR.002A

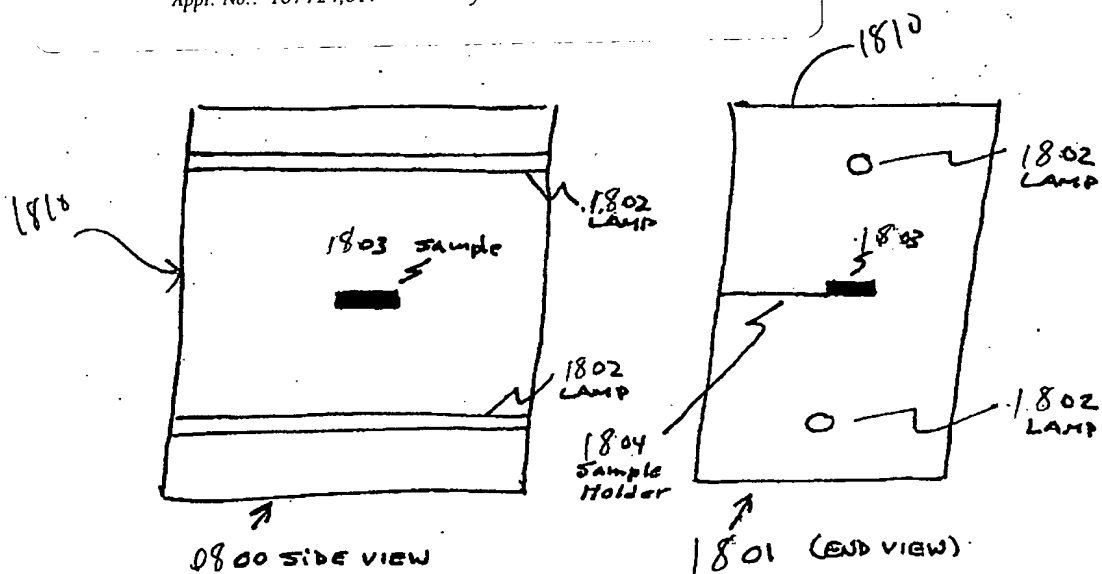


FIG 17A

FIG 17B

INTERNAL SAMPLE EXPOSURE SYSTEM

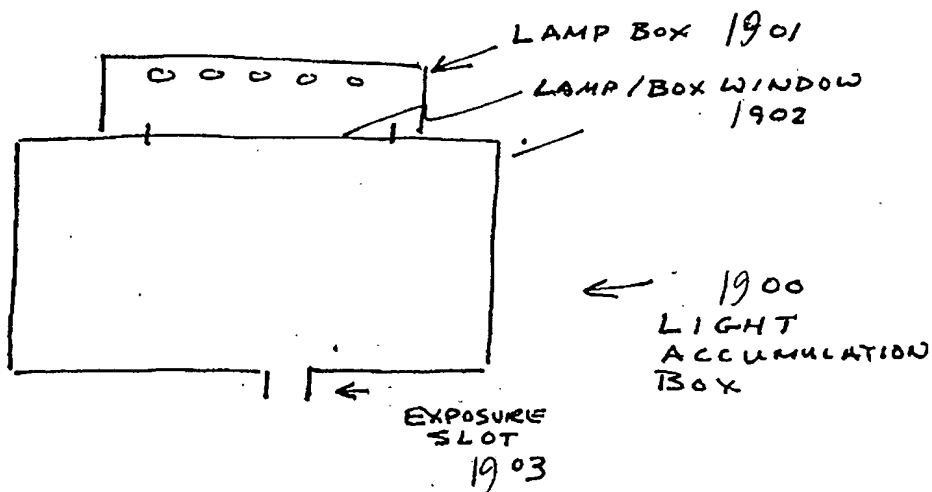


FIG. 18

UV Curing Model